

# Using the bq35100 with Li-Primary Based Applications



## 0.1 Why bq35100 ?

The BQ35100 is an accurate low power battery gauge that extends the life of primary batteries through accurate gauging. The gauge offers support for Lithium Thionyl Chloride chemistries with an EOS(end of service) algorithm which only consumes 0.35 uA of current as well as support for Lithium Manganese Dioxide chemistries with an SOH(state of health) algorithm which only consumes .06 uA of current. The device itself only needs to be powered long enough to record voltage, current, and temperature measurements used for computing parameters in SOH and EOS mode. These parameters, for instance, state of health and or impedance can be recorded based on user defined triggering of the GE pin which controls the devices power state. The user can obtain the results of EOS and SOH algorithms via an I2C bus, or use the ALERT output on the gauge as an interrupt to the host system. Additionally, the gauge algorithms support seamless replacement of old batteries and use an SHA-1 authentication to help prevent counterfeit battery usage. This gauge is best suited for use in products such as smoke alarms, flow meters, door access controllers, and similar devices for early fault detection and to maximize runtime.

## 0.2 Hardware

- EV2400 (Used for communicating over I2C with the BQ35100 IC)
- Power Supply (This can be a battery or power supply, the board is powered from this)
- USB 2.0 Type A to Type B (Connect EV2400 to your PC) I2C data cable (Connect EV2400 to board)

## 0.3 Software

- bqStudio Software (Program to interface with IC)
- EV2400 Firmware (Firmware for the 2400 must be updated in order to be used)

## 0.4 EV2400 Setup

- Connect usb from EV2400 to computer and connect data cable from EV2400 to I2C port

on the board.

- Connect your EV2400 to your PC and navigate to <http://www.ti.com/tool/EV2400> .
- Download the firmware and execute it in order to update your EV2400.

## 0.5 bqStudio Setup

- Navigate to <http://www.ti.com/tool/BQSTUDIO> and install the software.

## 0.6 Board Setup

- Place Jumpers across ALERT/PULL-UP
- Place Jumpers across GE/PULL-UP (Toggling this turns the device on and off)
- For one cell place jumpers across bottom two "1s".
- For multi-cell you will need to place jumpers on the top two 2-4s pins on J2.
- Following this place pins on J3 indicating the number of cells you have.
- Connect your battery across BAT+ and BAT-
- Connect data cable on J1 to the I2C port on your EV2400.

## 0.7 Loading Board Firmware (Optional)

- If your board does not come loaded with firmware or you wish to change it. Navigate to the Programming tab at the top.
- Select your .srec file and press PROGRAM. Once programming has finished press Execute FW. See "Programming" image in the Graphics section for reference.

## 0.8 Starting bqStudio

- Turn on your power supply and make sure you have jumped the GE pin.
- Upon launching bqStudio the software should auto detect the IC you are using. See "Start Screen" in the Graphics section for reference.
- You can use the SCAN button to continuously sample the visible parameters or use REFRESH at your discretion.

## 0.9 Using bqStudio

1. Press UNSEAL in the Commands tab. Check SEC1 and SEC0 in the Bit Registers window to see that SEC1 is green and SEC0 is red. (10) which means that the device has been unsealed
2. Press RESET in the Commands tab.
3. Press CAL\_TOGGLE in the Commands tab.
4. If you are using a pack with more than one cell in series, navigate to the gas gauging tab within the Data Memory tab. Make sure to enter your series cell count and write it the data flash prior to calibration. See "Series Cell Count" in the Graphics section for reference.
5. Navigate to the calibration tab at the top.
6. Check the "calibrate voltage" box and enter the measured voltage. You may get an error related to scanning in which navigate back to the Registers tab and turn scanning off. Once voltage calibration is finished uncheck the box next to it.
7. Repeat this procedure for the current and the temperature.
8. Finally, check Calibrate CC Offset and calibrate.
9. In the Command tab press CAL\_TOGGLE so that CalMode in the Bit Registers is Green indicating 0 which is off.

## 0.10 Cell Chemistry

- Navigate to the Chemistry tab.
- When selecting the Chem ID, primary cell IDs are listed as 6xxx. If you cannot find your specific model contact Texas Instruments on model generation.
- Select the chemistry you are using and press Program selected chemistry. See "Cell Chemistry" in the Graphics section for reference.

## 0.11 Entering Into SOH Mode

This mode is used for tracking capacity of batteries where the capacity decreases steadily with no sharp increases in internal impedance. Moreover this is characteristic of Lithium Manganese Dioxide chemistries.

1. Press UNSEAL in the COMMAND tab. Check SEC1 and SEC0
2. Press NEW\_BATTERY in the Commands tab.

3. Navigate to the Data Memory tab.
4. In the Data Memory tab press on the Configuration button.
5. From here press on "Operation Config A".
6. Observe the values of Bit1 (GMSEL1) and Bit0(GMSEL0). To be in SOH mode we need the values to be as such GMSEL1 = 0 =green and GMSEL0 = 1 = red. Press on GMSEL0 so that it turns red and changes what mode we are in and save. Reference the "GM Select" image in the Graphics section for where you should be when changing GM Sel.(NOTE: In the referenced image the operating mode is set to EOS)
7. We are now in SOH mode.
8. Navigate to Gas Gauging in the sidebar. Here are variables the user can modify as needed. Here you can enter the series cell count, etc.
9. Once you SOH decrease it will not increase so you will need to press NEW\_BATTERY each time you wish to use a new cell.

### 0.11.1 SOH Mode Fundamentals

SOH mode takes in the battery voltage and temperature. The gauge uses these two values and references them to the OCV lookup table in order to determine the SOH. One important variable to adjust in the Gas Gauging sidebar is the "State of Health Max Delta". This variable determines by how much you SOH can change with every cycle of the GE pin. If you plan on sampling very frequently and reading the voltage lower values will work. However, if your delta value is low and the voltage drops very suddenly you will not observe a change immediately but rather it will take multiple cycles to catch up to the new voltage.

### 0.11.2 Using SOH Mode

Once you have followed the above steps, using SOH mode is simple. Have your battery connected to the gauge and simply cycle the GE pin in order to get updated values of SOH after you have finished loading and the battery's open circuit voltage has relaxed back up. It is essential to wait for the battery's open circuit voltage to relax up in order to get accurate SOH readings. Make sure to press NEW\_BATTERY if you are inserting a new cell.

## 0.12 Entering Into EOS Mode

EOS is used for devices where the overall capacity doesn't decrease steadily with time but rather drops off sharply at the end of its life due to a sharp increase in impedance. Moreover this is characteristic of Lithium Thionyl Chloride chemistries. Reference the "Battery Impedance at EOS" graph on the Graphics page to see a characteristic curve of impedance increasing at EOS.

1. Press UNSEAL in the COMMAND tab. Check SEC1 and SEC0
2. Press NEW\_BATTERY in the Commands tab.
3. Navigate to the Data Memory tab.
4. In the Data Memory tab press on the Configuration button.
5. From here press on "Operation Config A".
6. Observe the values of Bit1 (GMSEL1) and Bit0(GMSEL0). To be in EOS mode we need the values to be as such GMSEL1 = 1=red and GMSEL0 = 0 = green. Press on GMSEL1 so that it turns red and changes what mode we are in and save.
7. We are now in EOS mode.
8. Navigate to the EOSData tab, here there are important variables the user can modify which will be subsequently discussed.

### 0.12.1 EOS Mode Fundamentals

EOS mode works by tracking the internal impedance of your battery with a short trend and long trend average. The gauge looks for a sharp increase in the short trend average when compared to the long trend average. The EOS Trend Detection average is the % increase of the short trend average in relation to the long trend average. Once the equation below is satisfied an EOS condition is set in the Battery Alert register. Reference the "EOS Usage" diagram on the Graphics page for a flowchart on using the mode.

$$\text{Short Trend Average} > \text{Long Trend Average} * (1 + \text{EOS Trend Detection} / 100)$$

### 0.12.2 Using EOS Mode

One important parameter to consider is the EOS Detection Pulse Count Thrshd. This threshold is the number of Gauge\_Start and Gauge\_Stop cycles you must perform before your device will begin calculating the short trend

and long trend averages for EOS detection. Adjust this value in accordance with how many times you will cycle your device. Modify the trend detection value based on how sharp of a decline your battery exhibits during EOS. Additionally make sure to adjust your cell terminate value under the Gas Gauging tab. Values for the impedance and SOH become available after the G\_DONE bit is set to 1. Reference the "EOS Usage" diagram in the Graphics section for a flowchart on using the mode as well as the "EOS Parameters" image in the Graphics section for modifiable parameters.

## 0.13 When is my battery empty?

When using EOS or SOH mode it is important to understand when a battery is dead. In general, a battery is considered dead when the relaxed open circuit voltage is at or below the terminate voltage. In SOH mode the decline towards this voltage is easy to see with each successive discharge bringing the relaxed voltage closer to the terminate voltage. Towards the end of a batteries life in SOH mode, the voltage will begin to dip to or below the terminate voltage and relax up to subsequently lower values with successive discharges. With EOS mode, the sharp increase in impedance signals that the battery is close to being unusable and the battery is said to be completely depleted when the voltage drops below the terminate voltage. This change happens rapidly and the battery itself becomes unusable very quickly.

## 1 Golden Image

Once you have calibrated, loaded the chemistry, and made sure your gauge is operating as you would like. You can extract a "golden image" file which is essentially an image of the flash memory that you can load into additional gauges so that you do not have to perform setup steps repeatedly. The "xxx.srec" file you extract can be used to program gauges as described in the "Loading Board Firmware Section". In order to extract the "xxx.srec" simply press "Create Image Files". See the "Golden Image" image in the Graphics section for further reference.

### 1.1 Trademarks

All trademarks are the property of their respective owners.

## 2 Advanced Programming

In the advanced programming tab you can send I2C commands to the gauge to read and write data. See the "Advanced Communications" image in the Graphics section for an example of requesting the voltage.

## 3 Related Documentation

For information regarding sending I2C commands to your device see the [Using I2C Communications Manual](#).

For more detailed information about the BQ35100 see the [Technical Reference Manual](#).

For more information about the EV2400 see the [EV2400 EVM Interface Board manual](#).

### 3.1 Trademarks

All other trademarks are the property of their respective owners.



## 1 Programming

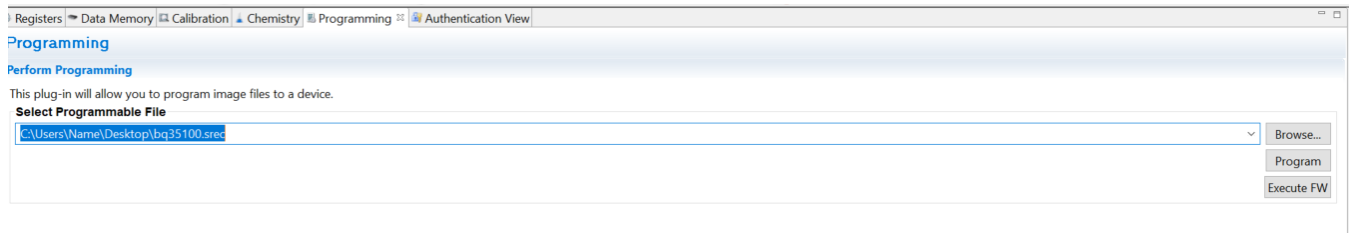


Figure 1. Programming xxx.srec file

## 2 Start Screen


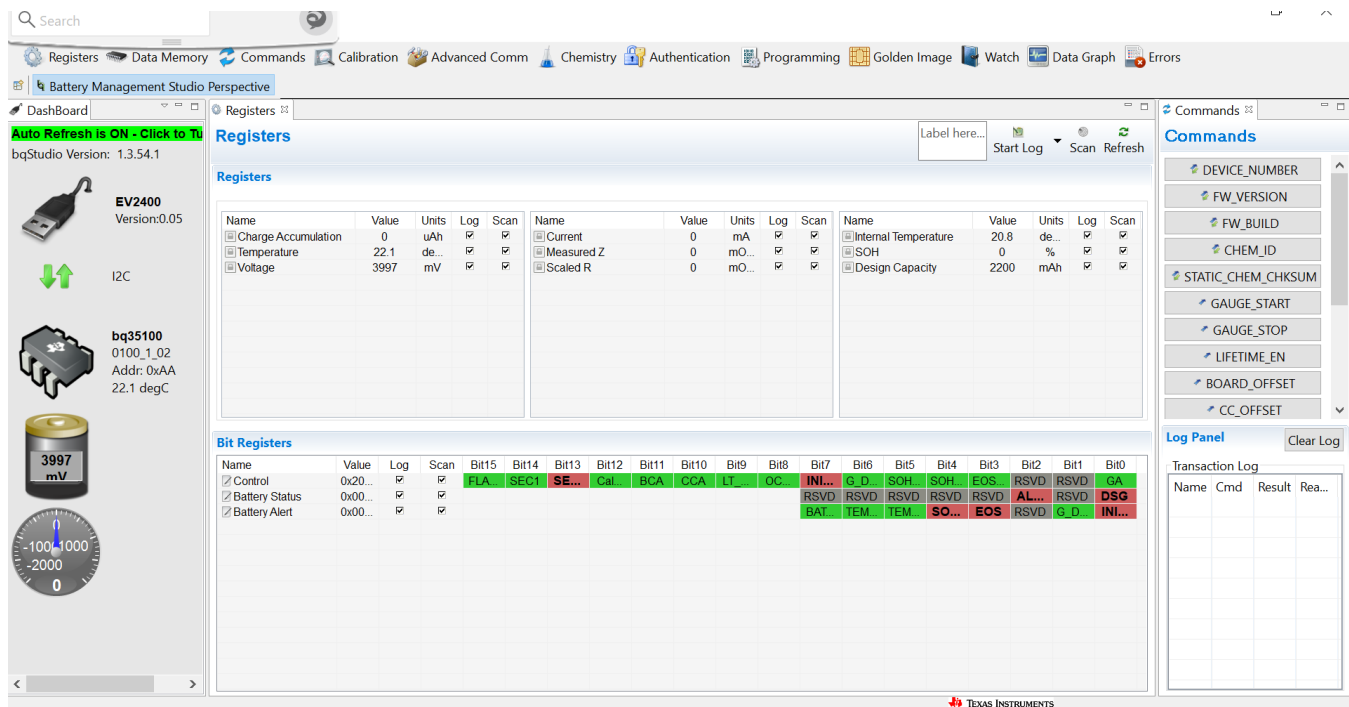


Figure 2. Start Screen

### Figure 3. Modifying series cell count in data flash


## 4 Calibration

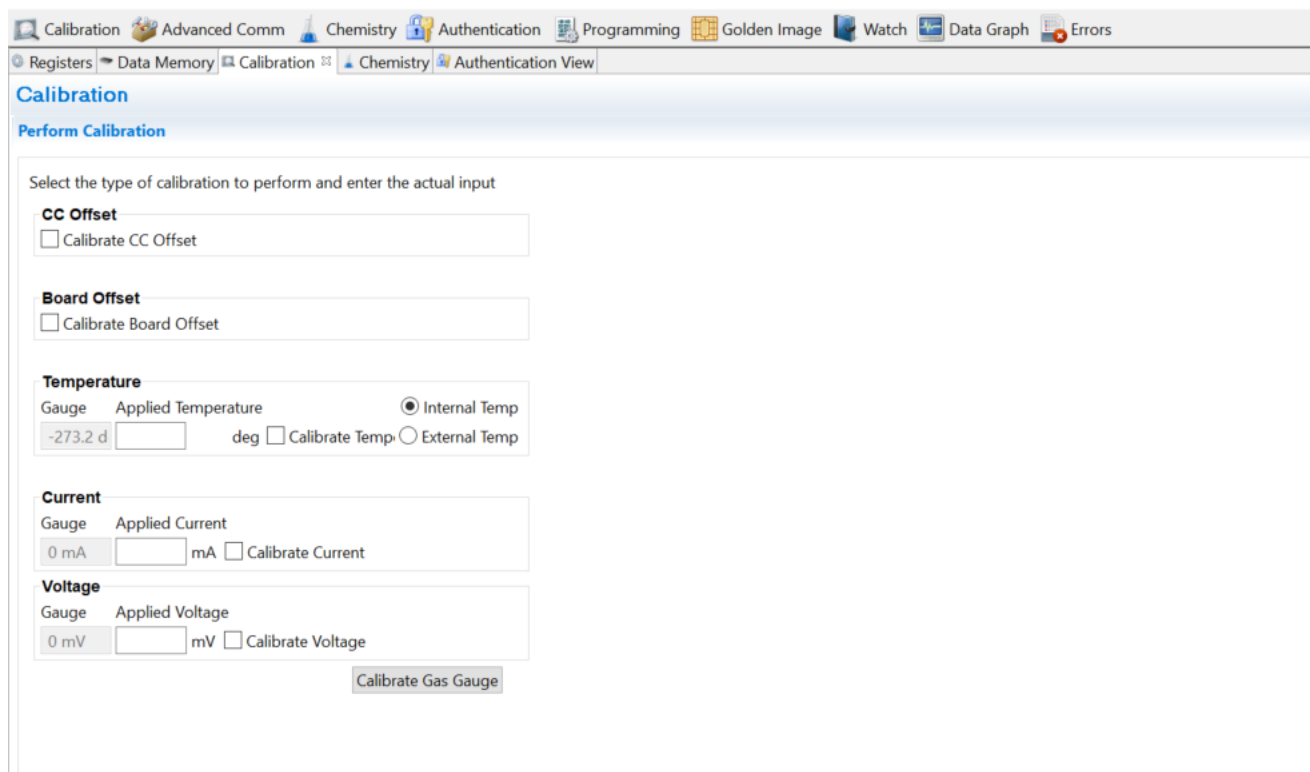

The Calibration screen in the Battery Management Studio software. It features a top toolbar with icons for Calibration, Advanced Comm, Chemistry, Authentication, Programming, Golden Image, Watch, Data Graph, and Errors. Below the toolbar is a navigation bar with tabs for Registers, Data Memory, Calibration (selected), Chemistry, and Authentication View. The main area is titled 'Calibration' and contains a 'Perform Calibration' section. This section prompts the user to 'Select the type of calibration to perform and enter the actual input'. It includes four main categories: CC Offset (with a checkbox for 'Calibrate CC Offset'), Board Offset (with a checkbox for 'Calibrate Board Offset'), Temperature (with radio buttons for 'Gauge', 'Applied Temperature', and 'Internal Temp' (selected), and a text input for '-273.2 d' and a checkbox for 'Calibrate Temp'), and Current (with radio buttons for 'Gauge' and 'Applied Current', and a text input for '0 mA' and a checkbox for 'Calibrate Current'). There is also a 'Voltage' section with radio buttons for 'Gauge' and 'Applied Voltage', and a text input for '0 mV' and a checkbox for 'Calibrate Voltage'. A 'Calibrate Gas Gauge' button is located at the bottom right of the main area.

Figure 4. Calibration Screen

## 5 Cell Chemistry

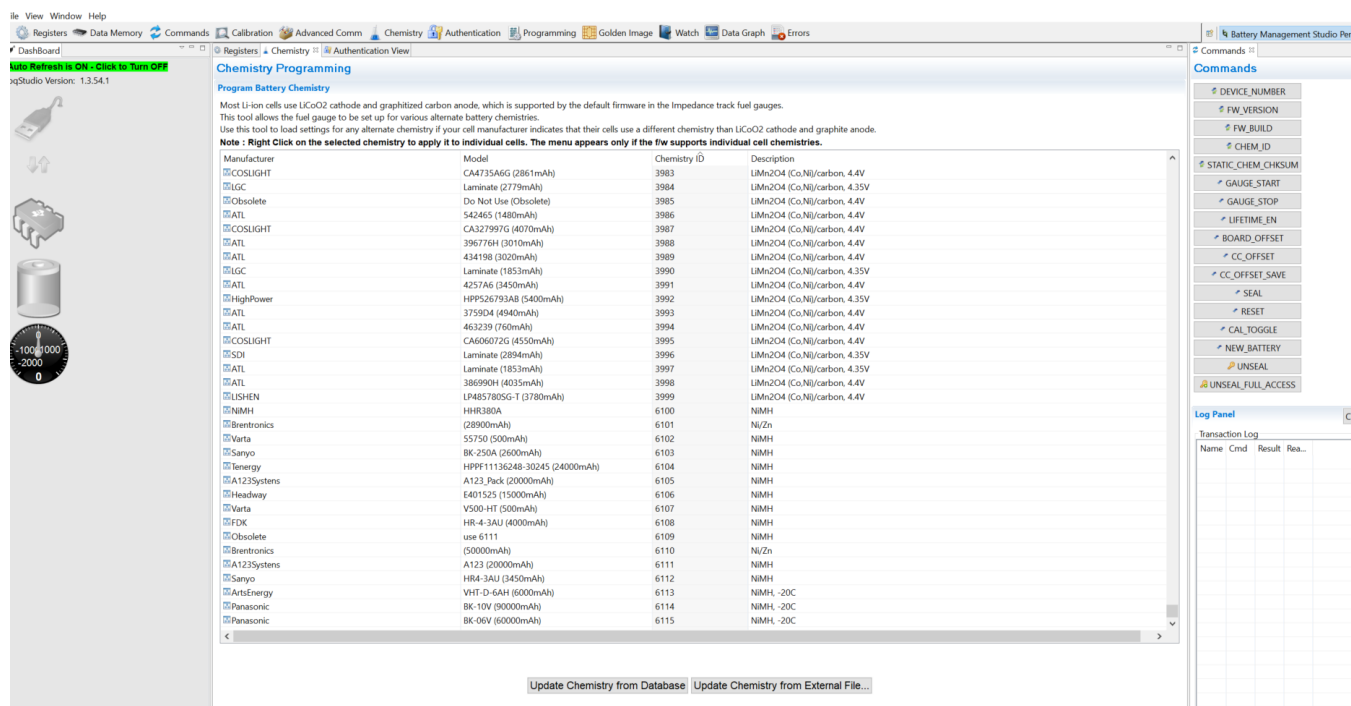

The Chemistry Programming screen in the Battery Management Studio software. It features a top toolbar with icons for Registers, Data Memory, Commands, Calibration, Advanced Comm, Chemistry (selected), Authentication, Programming, Golden Image, Watch, Data Graph, and Errors. Below the toolbar is a navigation bar with tabs for Registers, Chemistry (selected), and Authentication View. The main area is titled 'Chemistry Programming' and contains a 'Program Battery Chemistry' section. This section includes a text area with instructions: 'Most Li-ion cells use LiCoO2 cathode and graphitized carbon anode, which is supported by the default firmware in the Impedance track fuel gauges. This tool allows the fuel gauge to be set up for various alternate battery chemistries. Use this tool to load settings for any alternate chemistry if your cell manufacturer indicates that their cells use a different chemistry than LiCoO2 cathode and graphite anode. Note: Right Click on the selected chemistry to apply it to individual cells. The menu appears only if the fw supports individual cell chemistries.' Below this is a table with columns for Manufacturer, Model, Chemistry ID, and Description. The table lists various manufacturers and their corresponding models and chemistry IDs. At the bottom of the table are two buttons: 'Update Chemistry from Database' and 'Update Chemistry from External File...'. On the right side of the screen is a 'Commands' panel with a list of commands: DEVICE\_NUMBER, FW\_VERSION, FW\_BUILD, CHEM\_ID, STATIC\_CHEM\_CHKSUM, GAUGE\_START, GAUGE\_STOP, LIFETIME\_EN, BOARD\_OFFSET, CC\_OFFSET, CC\_OFFSET\_SAVE, SEAL, RESET, CAL\_TOGGLE, NEW\_BATTERY, UNSEAL, and UNSEAL\_FULL\_ACCESS. Below the commands panel is a 'Log Panel' with a 'Transaction Log' table showing Name, Cmd, Result, and Rea... columns.

Figure 5. Chemistry Programming Screen



## 6 GM Select

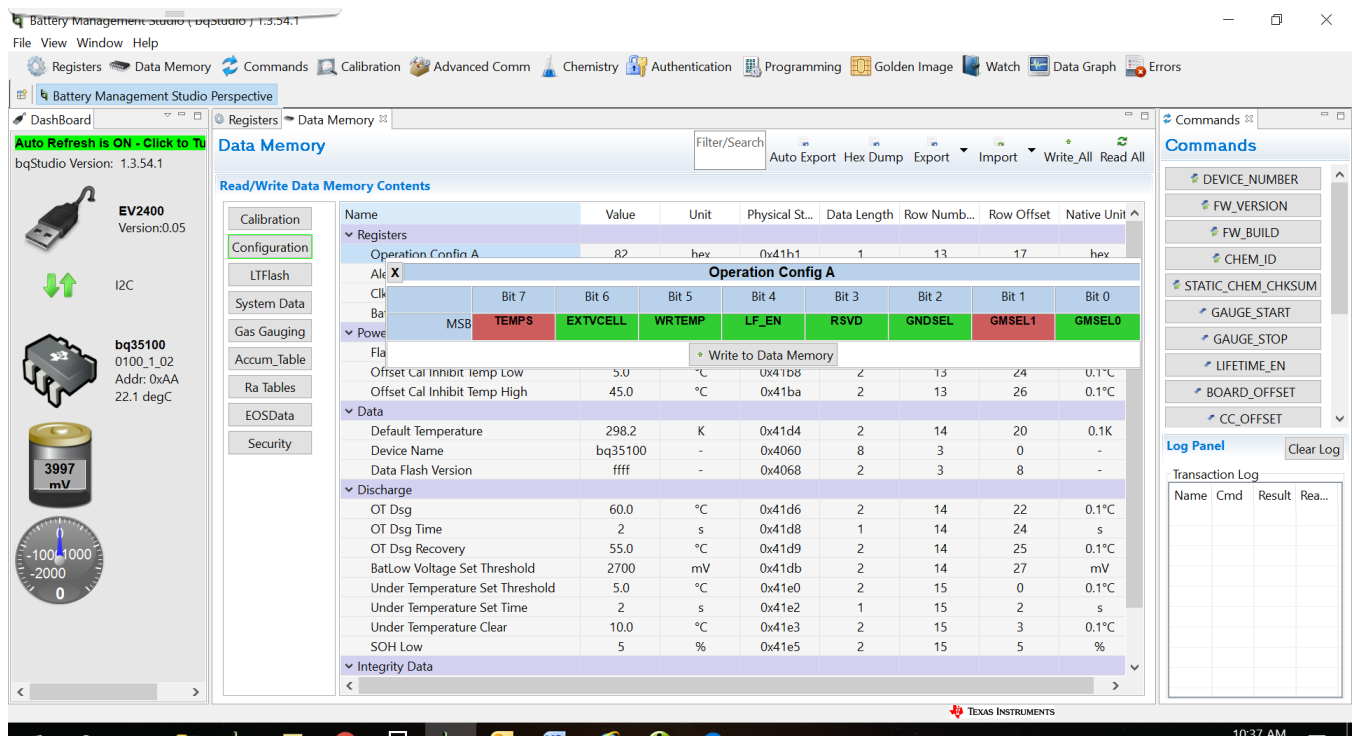


Figure 6. GM select is toggled to change operating modes in this image the operating mode is set to EOS

## 7 SOH Usage

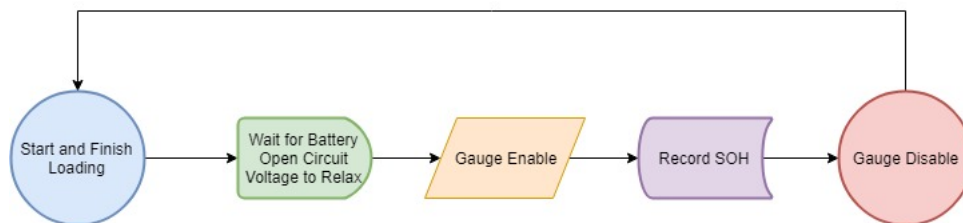


Figure 7. SOH Mode Usage Diagram



## 8 EOS Parameters

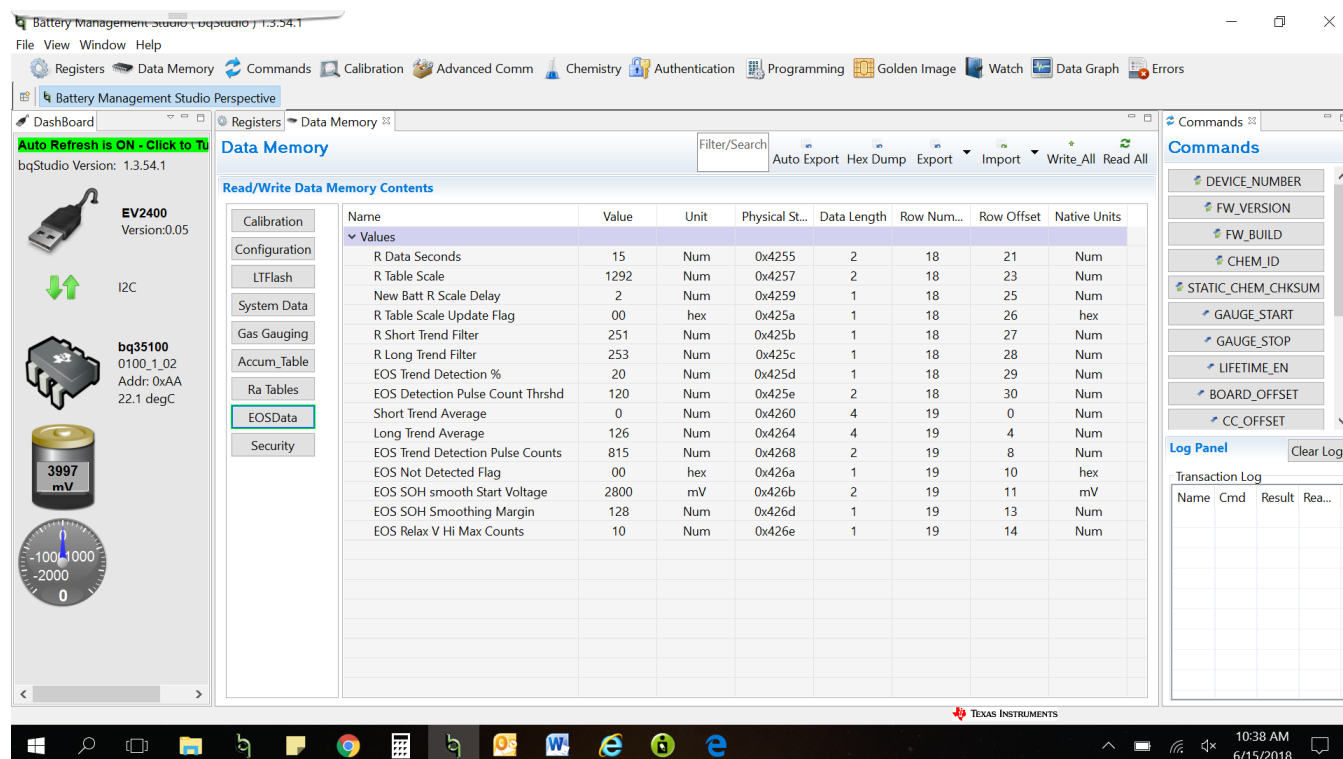


Figure 8. EOS parameters that can be modified

## 9 EOS Usage

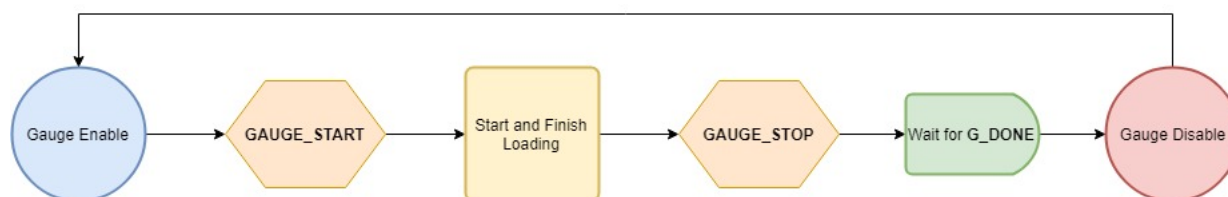


Figure 9. EOS Mode Usage Diagram

## 10 Battery Impedance at EOS

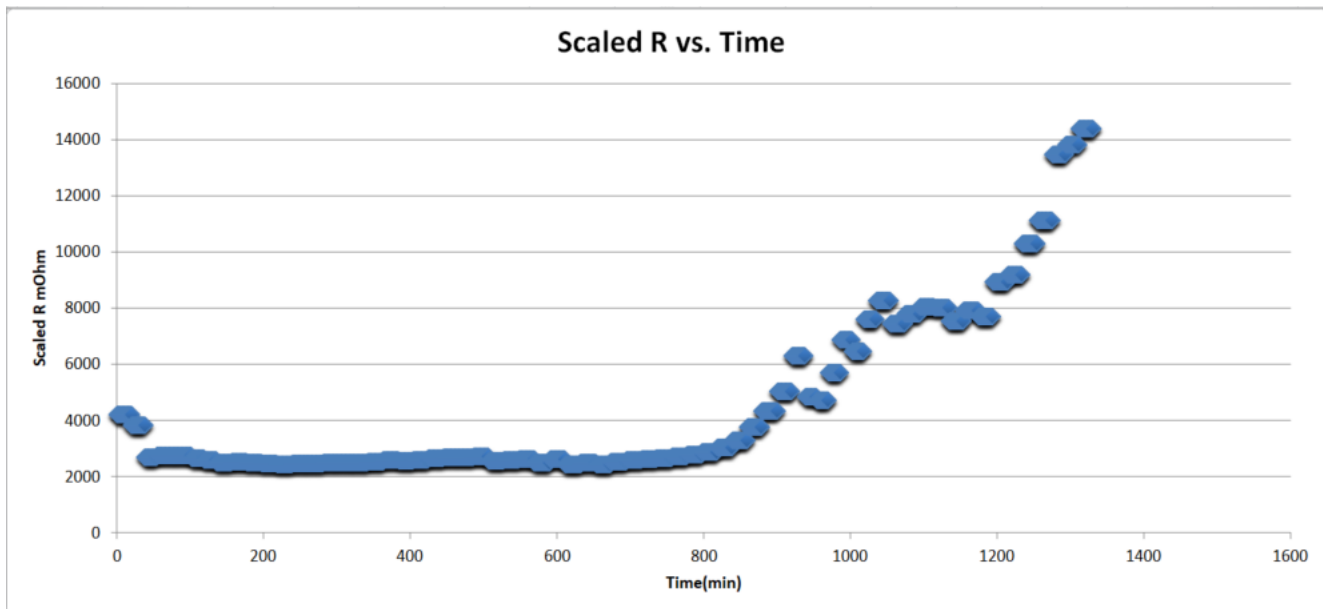


Figure 10. Scaled-R increasing at EOS

## 11 Golden Image

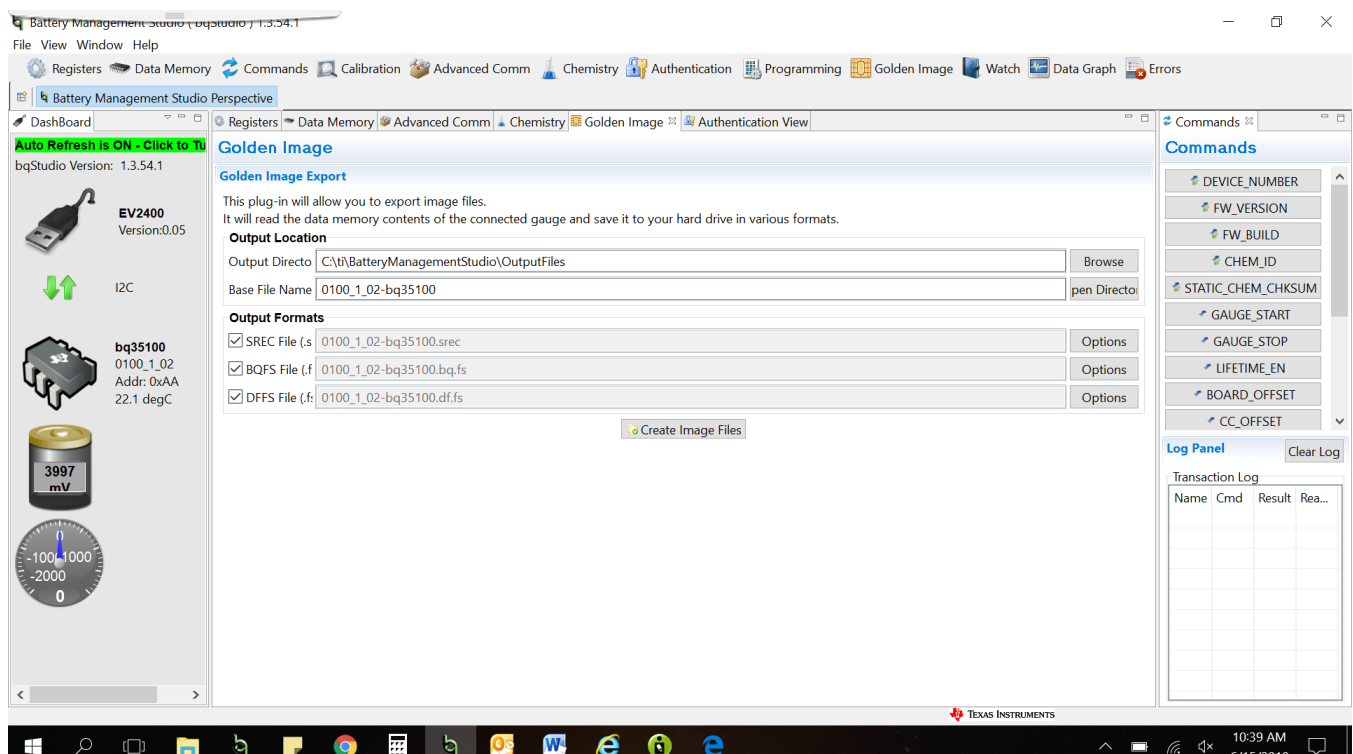


Figure 11. Golden image extraction



## IMPORTANT NOTICE FOR TI DESIGN INFORMATION AND RESOURCES

Texas Instruments Incorporated ("TI") technical, application or other design advice, services or information, including, but not limited to, reference designs and materials relating to evaluation modules, (collectively, "TI Resources") are intended to assist designers who are developing applications that incorporate TI products; by downloading, accessing or using any particular TI Resource in any way, you (individually or, if you are acting on behalf of a company, your company) agree to use it solely for this purpose and subject to the terms of this Notice.

TI's provision of TI Resources does not expand or otherwise alter TI's applicable published warranties or warranty disclaimers for TI products, and no additional obligations or liabilities arise from TI providing such TI Resources. TI reserves the right to make corrections, enhancements, improvements and other changes to its TI Resources.

You understand and agree that you remain responsible for using your independent analysis, evaluation and judgment in designing your applications and that you have full and exclusive responsibility to assure the safety of your applications and compliance of your applications (and of all TI products used in or for your applications) with all applicable regulations, laws and other applicable requirements. You represent that, with respect to your applications, you have all the necessary expertise to create and implement safeguards that (1) anticipate dangerous consequences of failures, (2) monitor failures and their consequences, and (3) lessen the likelihood of failures that might cause harm and take appropriate actions. You agree that prior to using or distributing any applications that include TI products, you will thoroughly test such applications and the functionality of such TI products as used in such applications. TI has not conducted any testing other than that specifically described in the published documentation for a particular TI Resource.

You are authorized to use, copy and modify any individual TI Resource only in connection with the development of applications that include the TI product(s) identified in such TI Resource. NO OTHER LICENSE, EXPRESS OR IMPLIED, BY ESTOPPEL OR OTHERWISE TO ANY OTHER TI INTELLECTUAL PROPERTY RIGHT, AND NO LICENSE TO ANY TECHNOLOGY OR INTELLECTUAL PROPERTY RIGHT OF TI OR ANY THIRD PARTY IS GRANTED HEREIN, including but not limited to any patent right, copyright, mask work right, or other intellectual property right relating to any combination, machine, or process in which TI products or services are used. Information regarding or referencing third-party products or services does not constitute a license to use such products or services, or a warranty or endorsement thereof. Use of TI Resources may require a license from a third party under the patents or other intellectual property of the third party, or a license from TI under the patents or other intellectual property of TI.

TI RESOURCES ARE PROVIDED "AS IS" AND WITH ALL FAULTS. TI DISCLAIMS ALL OTHER WARRANTIES OR REPRESENTATIONS, EXPRESS OR IMPLIED, REGARDING TI RESOURCES OR USE THEREOF, INCLUDING BUT NOT LIMITED TO ACCURACY OR COMPLETENESS, TITLE, ANY EPIDEMIC FAILURE WARRANTY AND ANY IMPLIED WARRANTIES OF MERCHANTABILITY, FITNESS FOR A PARTICULAR PURPOSE, AND NON-INFRINGEMENT OF ANY THIRD PARTY INTELLECTUAL PROPERTY RIGHTS.

TI SHALL NOT BE LIABLE FOR AND SHALL NOT DEFEND OR INDEMNIFY YOU AGAINST ANY CLAIM, INCLUDING BUT NOT LIMITED TO ANY INFRINGEMENT CLAIM THAT RELATES TO OR IS BASED ON ANY COMBINATION OF PRODUCTS EVEN IF DESCRIBED IN TI RESOURCES OR OTHERWISE. IN NO EVENT SHALL TI BE LIABLE FOR ANY ACTUAL, DIRECT, SPECIAL, COLLATERAL, INDIRECT, PUNITIVE, INCIDENTAL, CONSEQUENTIAL OR EXEMPLARY DAMAGES IN CONNECTION WITH OR ARISING OUT OF TI RESOURCES OR USE THEREOF, AND REGARDLESS OF WHETHER TI HAS BEEN ADVISED OF THE POSSIBILITY OF SUCH DAMAGES.

You agree to fully indemnify TI and its representatives against any damages, costs, losses, and/or liabilities arising out of your non-compliance with the terms and provisions of this Notice.

This Notice applies to TI Resources. Additional terms apply to the use and purchase of certain types of materials, TI products and services. These include; without limitation, TI's standard terms for semiconductor products (<http://www.ti.com/sc/docs/stdterms.htm>), [evaluation modules](#), and [samples](http://www.ti.com/sc/docs/sampterm.htm) (<http://www.ti.com/sc/docs/sampterm.htm>).

Mailing Address: Texas Instruments, Post Office Box 655303, Dallas, Texas 75265  
Copyright © 2018, Texas Instruments Incorporated